



Rewarding Learning

ADVANCED

General Certificate of Education

2019

Centre Number

| | | | | |
|--|--|--|--|--|
| | | | | |
|--|--|--|--|--|

Candidate Number

| | | | |
|--|--|--|--|
| | | | |
|--|--|--|--|

Life and Health Sciences

Assessment Unit A2 3

assessing

Medical Physics

[AZ031]

FRIDAY 31 MAY, AFTERNOON



AZ031

TIME

1 hour 45 minutes.

INSTRUCTIONS TO CANDIDATES

Write your Centre Number and Candidate Number in the spaces provided at the top of this page.

Write your answers in the spaces provided in this question paper.

Answer **all eight** questions.

INFORMATION FOR CANDIDATES

The total mark for this paper is 100.

Figures in brackets printed down the right-hand side of pages indicate the marks awarded to each question or part question.

You may use an electronic calculator.

Quality of written communication will be assessed in question **1(ii)**.

| For Examiner's use only | |
|-------------------------|-------|
| Question Number | Marks |
| 1 | |
| 2 | |
| 3 | |
| 4 | |
| 5 | |
| 6 | |
| 7 | |
| 8 | |

| | |
|--------------------|--|
| Total Marks | |
|--------------------|--|

[8]

| Examiner Only | |
|---------------|--------|
| Marks | Remark |
| | |

2 Table 2.1 shows data for some radioisotopes.

Table 2.1

| Isotope | Half-life / days | | |
|------------------|-----------------------|-------------------------|------------------------|
| | T_{Physical} | $T_{\text{Biological}}$ | $T_{\text{Effective}}$ |
| ^{90}Sr | 1.1×10^4 | 1.8×10^4 | |
| ^{32}P | 14.3 | 1155 | 14.1 |
| ^{131}I | 8 | 135 | 7.55 |

The rate of decrease of radiation exposure is affected by both the radioactive half-life, T_{Physical} , and biological half-life, $T_{\text{Biological}}$, giving an effective half-life, $T_{\text{Effective}}$, for the isotope in the body.

(a) Explain why it is important that a patient has minimal exposure to a radioisotope.

[2]

Phosphorus, ^{32}P , and strontium, ^{90}Sr , are **both taken up by bone**.

(b) (i) Describe and explain the effects this will have, if any, on the radioactive half-life, T_{Physical} , and on the biological half-life, $T_{\text{Biological}}$.

T_{Physical} _____

[2]

$T_{\text{Biological}}$ _____

[2]

Examiner Only

Marks Remark

From the examples shown in **Table 2.1**, it can be observed that sometimes biological half-life is the dominant influence and sometimes physical half-life is the dominant influence.

Equation 2.1 below is used to calculate the effective half-life for a radioisotope.

$$\frac{1}{T_{\text{Effective}}} = \frac{1}{T_{\text{Physical}}} + \frac{1}{T_{\text{Biological}}} \quad \text{Equation 2.1}$$

- (ii) Using data from **Table 2.1**, calculate the effective half-life, $T_{\text{effective}}$, for ^{90}Sr .

You are advised to show your working.

Effective half-life for ^{90}Sr = _____ days
[3]

- (iii) Evaluate which of the two radioisotopes, ^{90}Sr or ^{32}P , would be safer to use in bone scans.

[3]

| Examiner Only | |
|---------------|--------|
| Marks | Remark |
| | |

- 3 Under normal circumstances the human body maintains a constant temperature called core temperature.

A lowering of body temperature is known as hypothermia and a raising of body temperature is known as hyperthermia.


- (a) (i) What is the value of the core temperature?

_____ °C [1]

- (ii) What are the temperatures above and below which the human body can no longer stay alive?

Above _____ °C Below _____ °C [2]

- (b) Fig. 3.1 below shows 3 different types of thermometer which can be used to measure body temperature.

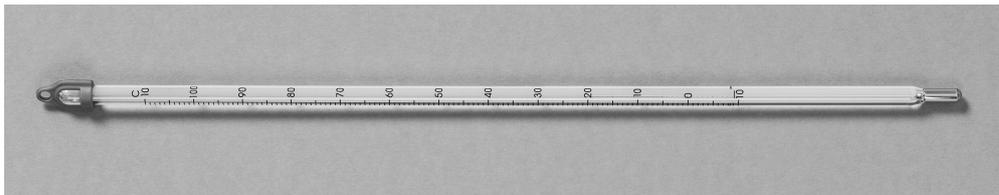

Mercury in glass thermometer



Digital thermometer



Electronic thermometer

Source: Principal Examiner

Fig. 3.1

| Examiner Only | |
|---------------|--------|
| Marks | Remark |
| | |

- (i) Complete **Table 3.1** to give one method of use and one limitation for each of these thermometers.
Write your answers in the blank boxes below.

Table 3.1

| Type of Thermometer | Method of use | Limitation |
|------------------------------|---------------|------------|
| Mercury in glass thermometer | | |
| Digital thermometer | | |
| Electronic thermometer | | |


[6]

- (ii) Mercury in glass thermometers are no longer commonly used by medical professionals to measure body temperature. Suggest a reason why they are considered unsafe to use for this purpose.

_____ [1]

| Examiner Only | |
|---------------|--------|
| Marks | Remark |
| | |

An electrocardiogram (ECG) works by measuring pulses of electric current flowing in the heart. These electrical impulses are then recorded as special tracings on strips of graph paper as seen in **Fig. 4.1**.

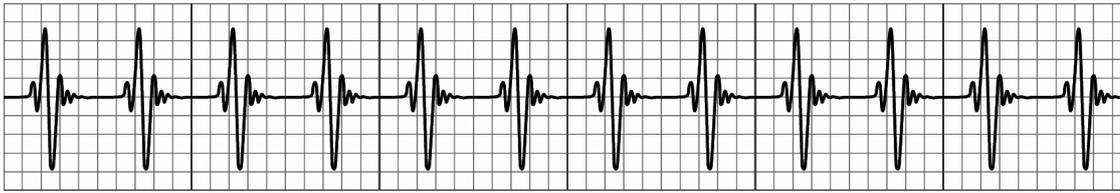

© AlexanderZam / Getty Images

Fig. 4.1

Long QT syndrome is a genetic heart condition which causes problems with the electrical activity of the heart.

It causes short episodes of abnormally fast heart rhythm which last for about a minute.

This can be triggered by stimuli such as stress, sudden noises, strenuous exercise and even sleeping.

(b) (i) State **two** other medical abnormalities which may be detected through the use of an electrocardiogram.

1. _____

2. _____
_____ [2]

(ii) Describe the limitations of an ECG when used to determine if a patient has long QT syndrome.

_____ [2]

Examiner Only

Marks Remark

- 5 **Fig. 5.1** shows a simplified X-ray tube used in the production of conventional X-rays and CT scans.

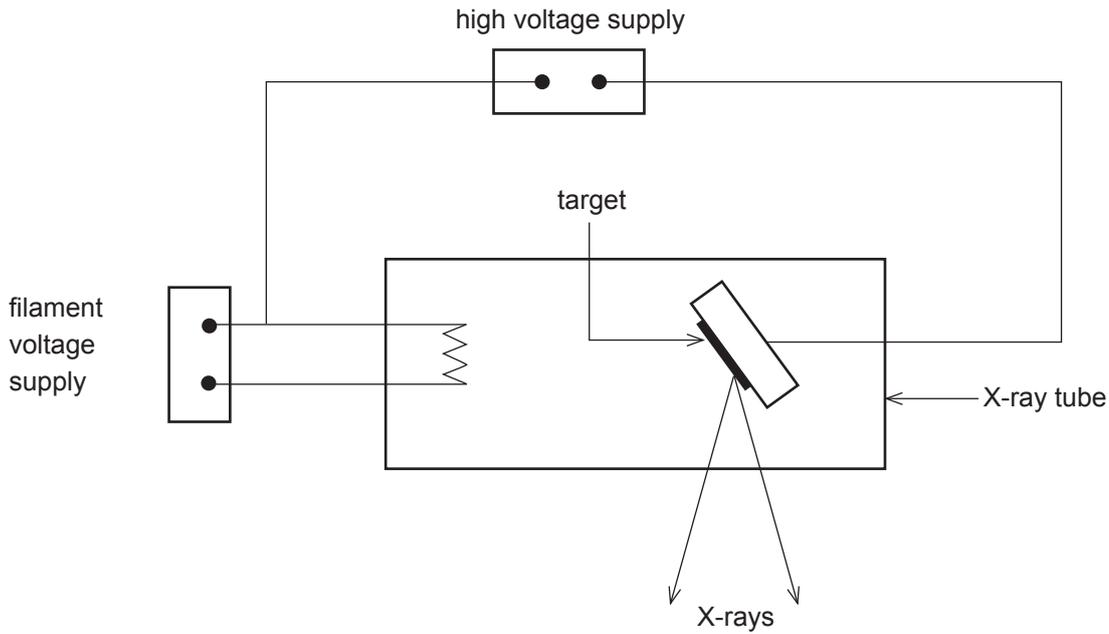


Fig. 5.1

- (a) (i) **Table 5.1** lists some possible properties of X-rays. Tick the appropriate boxes to indicate the correct properties of X-rays. One example has been provided.

Table 5.1

| Properties | |
|--|---|
| High energy wave | ✓ |
| Low frequency | |
| Cause ionisation of matter | |
| Has a relative charge of -1 | |
| Can travel in a vacuum | |
| Part of the electromagnetic spectrum | |
| Can only travel a few centimetres in air | |

[3]

Examiner Only

Marks Remark

- 6 A technician carried out an experiment to determine the activity of a radioactive source, **A**. The results collected from this experiment are shown in **Table 6.1** below.

Table 6.1

| Reading | Number of counts in 2 minutes |
|---------|-------------------------------|
| 1 | 287 |
| 2 | 300 |
| 3 | 298 |

- (a) (i) Activity is measured in becquerels, Bq.

What is the meaning of **1 Bq**?

_____ [1]

- (ii) Using all the results in **Table 6.1**, calculate the activity when source **A** is present. Give your answer to 3 significant figures.

You are advised to show your working.

Activity = _____ Bq [3]

The technician then recorded the counts for the background radiation over the same period of time and calculated the background activity to be 0.37 Bq.

- (iii) What is background radiation?

 _____ [1]

- (iv) Calculate the activity of radioactive source, **A**.

Activity = _____ Bq [1]

Examiner Only

Marks Remark

7 (a) (i) What is ultrasound?

_____ [1]

(ii) Outline how ultrasound is used in medical diagnostics.

_____ [2]

(b) (i) State the frequency range used for the medical imaging of breast tissue.

_____ [1]

(ii) Explain why the frequency range stated in (b)(i) is used.

_____ [2]

(iii) Explain why the frequency range stated in (b)(i) is unsuitable for ultrasound imaging of a deep structure, such as a kidney.

_____ [1]

(iv) What is the purpose of a coupling agent between the skin and ultrasound probe?

_____ [1]

Examiner Only

Marks

Remark

MRI scans are becoming increasingly common.

(c) (i) What do the letters MRI mean?

_____ [1]

(ii) Which part of the electromagnetic spectrum is used in an MRI scan?

_____ [1]

(iii) Explain why a patient who has had a cardiac pacemaker fitted, may not have an MRI scan of the heart.

_____ [2]

(iv) Suggest a reason why babies are usually not given an MRI scan.

_____ [1]

Examiner Only

Marks Remark

- 8 (a) In a B-scan, a 2.2 MHz ultrasound beam travels at a speed of 1.5 km s^{-1} through soft tissue.

If the specific acoustic impedance of soft tissue is $1.63 \times 10^6 \text{ kg m}^{-2} \text{ s}^{-1}$, calculate the density of the soft tissue.

You are advised to show your working.

Density = _____ kg m^{-3} [4]

The specific acoustic impedance for some materials is provided in **Table 8.1**.

Table 8.1

| Material | Specific acoustic impedance/ $\text{kg m}^{-2} \text{ s}^{-1}$ |
|----------|--|
| Skin | 1.63×10^6 |
| Oil | 1.43×10^6 |
| Fat | 1.38×10^6 |
| Bone | 7.78×10^6 |
| Muscle | 1.70×10^6 |

Examiner Only

Marks Remark

- (b) (i) Calculate the intensity reflection coefficient at the fat–muscle interface.

You are advised to show your working.

Intensity reflection coefficient = _____ [3]

- (ii) Between which two materials, listed in **Table 8.1**, will the most ultrasound energy be lost by reflection at the interface between the materials?

Explain your answer.

Materials: _____

Explanation: _____

_____ [3]

- (iii) State what will happen to the ultrasound energy lost as the ultrasound passes through a layer of tissue.

_____ [1]

| Examiner Only | |
|---------------|--------|
| Marks | Remark |
| | |

- (c) (i) Compare the visual output and uses of ultrasonic A-scans and B-scans.

_____ [2]

- (ii) Which type of ultrasonic scan requires the operator to move the probe continuously across the surface of the skin?

_____ [1]

- (iii) In an A-scan of a tumour the time taken between the reflected pulses from each surface of the tumour is $60\ \mu\text{s}$. If the speed of ultrasound in the tumour is $1500\ \text{m s}^{-1}$, calculate the diameter of the tumour.

You are advised to show your working.

diameter = _____ m [5]

THIS IS THE END OF THE QUESTION PAPER

| Examiner Only | |
|---------------|--------|
| Marks | Remark |
| | |

Permission to reproduce all copyright material has been applied for.
In some cases, efforts to contact copyright holders may have been unsuccessful and CCEA
will be happy to rectify any omissions of acknowledgement in future if notified.